



TEMPO[®]

FOOD QUALITY AUTOMATION

Because you count



PIONEERING DIAGNOSTICS

SIMPLIFY YOUR LIFE

ONLY 1 CARD




HIGHLY FLEXIBLE!


- MANAGEMENT OF SURGE TESTING NEEDS
- FAST START FOR "LAST MINUTE" SAMPLES
- QUICK TECHNICAL TRAINING

ONLY **3** STEPS
as simple as 1, 2, 3!

1 Automated sample preparation of samples



2 Incubation in your standard incubators




3 Automated reading and recording



"WITH TEMPO,
I CAN TEST
ON DEMAND"

REDUCE

- WASTE
Protect the environment and be lean
- INCUBATOR SPACE
- SUBJECTIVITY

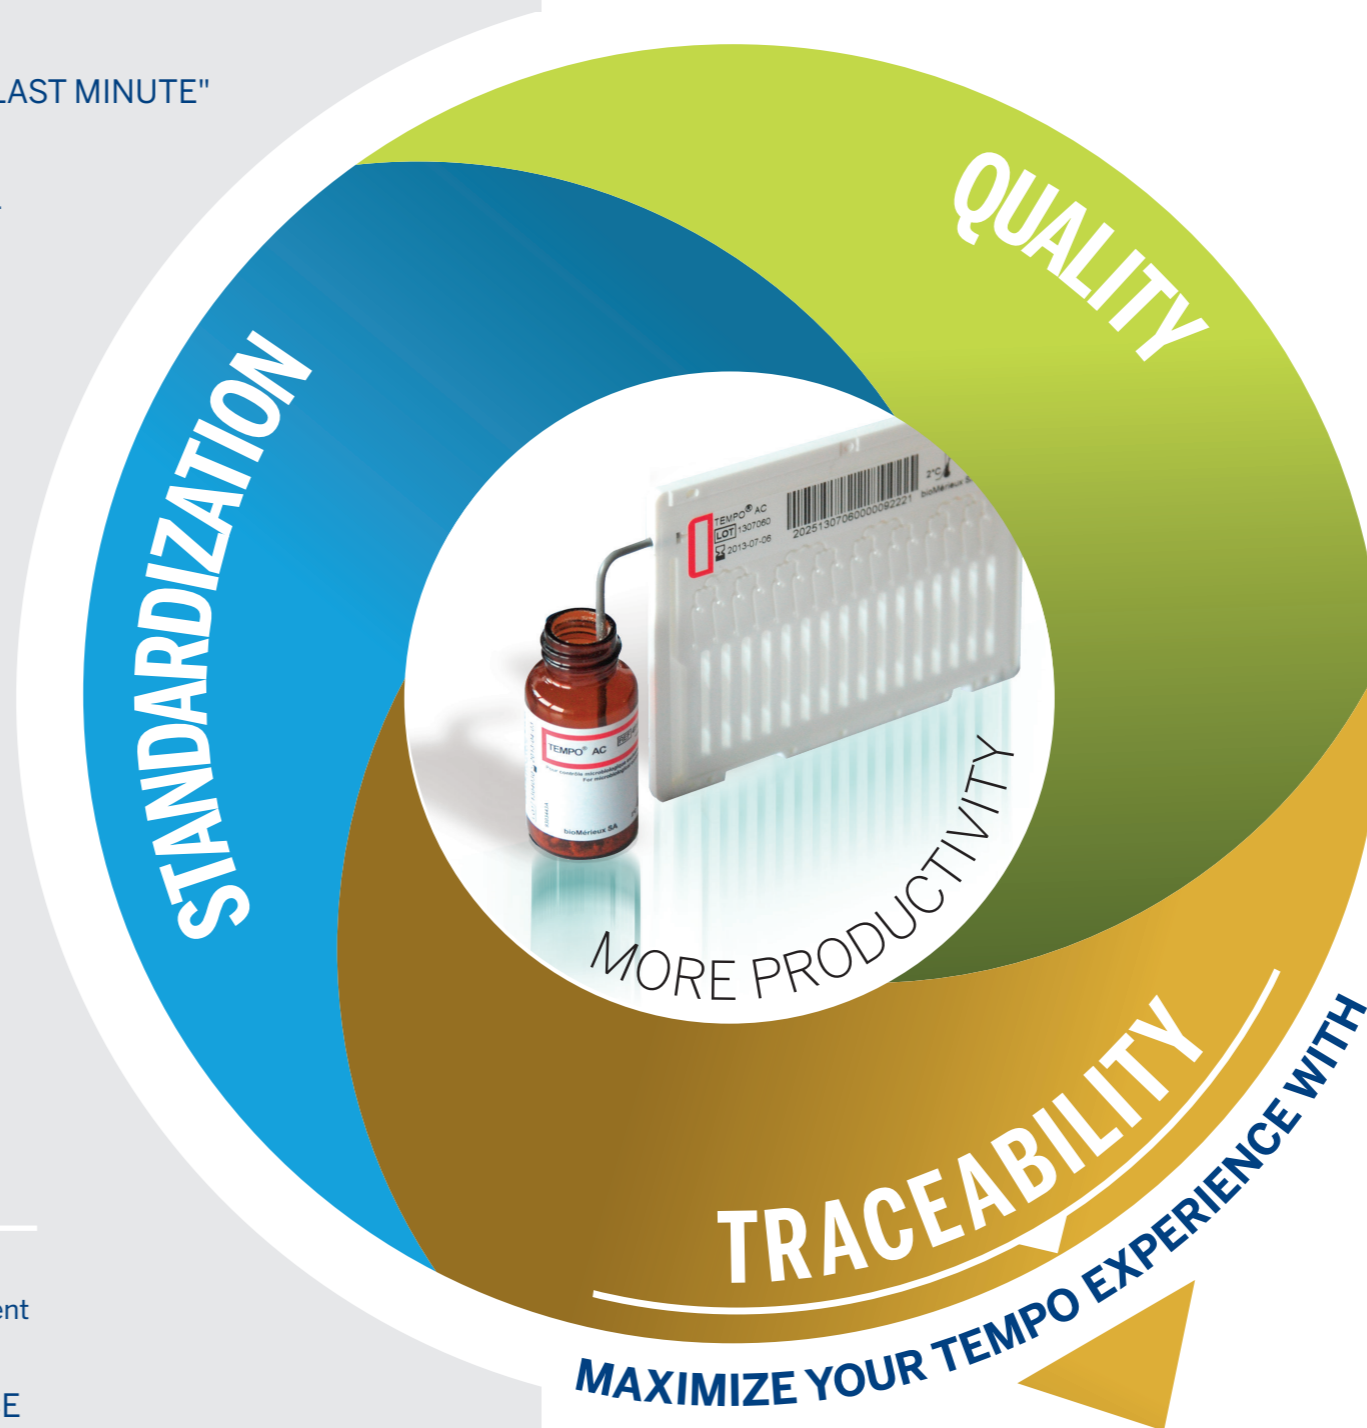

RESULTS YOU CAN COUNT ON

GLOBALY RECOGNIZED

- AFNOR & AOAC VALIDATED
- NO CROSS CONTAMINATION: SECURED PROTOCOL
- LONG SHELF LIFE REAGENTS

DATA INTEGRITY

KEEP YOUR DATA WITHIN COMPLIANCE STANDARDS

- FULL TRACEABILITY - INTEGRATED CONTROL PLAN & BARCODE
- SECURED DATA - FROM SAMPLE ID TO AUTOMATED RESULTS
- NO TRANSCRIPTION ERRORS

— bioMérieux —

CONNECT-UP™

MINIMIZE ADMINISTRATIVE TASKS,
GAIN ON VALUE-ADDED ACTIONS!



TEMPO® parameters


TEMPO parameters	NEXT DAY SOLUTION	AOAC	ISO
411113 AC <i>Aerobic mesophilic total flora</i>	✓	✓	✓
80002 STA <i>Staphylococcus (coag+)</i>	✓	✓	✓
80003 EB <i>Enterobacteriaceae</i>	✓	✓	✓
80004 EC <i>Escherishia coli</i>	✓	✓	✓
80006 TC <i>Coliforms</i>	✓		✓
80044 CC <i>Coliforms</i>	✓	✓	
80406 BC <i>Bacillus cereus</i>	✓	✓	✓
80001 YM <i>Yeast & Mold</i>	72-76 hr	✓	
80071 LAB <i>Lactic acid bacteria</i>	40-48 hr		
421509 CAM <i>Campylobacter</i>	48 hr		Coming soon!

GET THE RIGHT SOLUTION

SAMPLE PREPARATION



PRODUCTIVITY

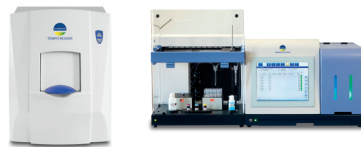

SAFETY



IDENTIFICATION

